



UNITED STATES PATENT AND TRADEMARK OFFICE

UNITED STATES DEPARTMENT OF COMMERCE
United States Patent and Trademark Office
Address: COMMISSIONER FOR PATENTS
P.O. Box 1450
Alexandria, Virginia 22313-1450
www.uspto.gov

BIBDATASHEET

CONFIRMATION NO. 4207

Bib Data Sheet

SERIAL NUMBER 10/613,117	FILING DATE 07/03/2003 RULE	CLASS 356	GROUP ART UNIT 2877	ATTORNEY DOCKET NO. LIFE-090CON4
-----------------------------	-----------------------------------	--------------	------------------------	-------------------------------------

APPLICANTS

John P. Sopp, White Bear Lake, MN;

Scott T. Latterell, Minneapolis, MN;

Paul D. Brinda, Robbinsdale, MN; Timothy J. Erskine, Sandy, UT;

** CONTINUING DATA *****

NY This application is a CON of 10/233,046 08/30/2002 PAT 6,624,882
which is a CON of 09/723,339 11/27/2000 PAT 6,614,522
which is a CON of 09/264,461 03/08/1999 PAT 6,152,889
which is a DIV of 08/706,663 09/06/1996 PAT 5,879,310
which is a CIP of 08/525,390 09/08/1995 ABN
and is a CIP of 08/525,942 09/08/1995 PAT 5,879,367

** FOREIGN APPLICATIONS *****

IF REQUIRED, FOREIGN FILING LICENSE GRANTED

** 10/01/2003

Foreign Priority claimed	<input type="checkbox"/> yes <input checked="" type="checkbox"/> no	STATE OR COUNTRY	SHEETS	TOTAL	INDEPENDENT
35 USC 119 (a-d) conditions met	<input type="checkbox"/> yes <input checked="" type="checkbox"/> no	Met after Allowance			
Verified and Acknowledged	<i>9/7/03</i>	Initials	DRAWING 28	CLAIMS 19	CLAIMS 2

ADDRESS

24353
BOZICEVIC, FIELD & FRANCIS LLP
1900 UNIVERSITY-AVE
SUITE 200
EAST PALO ALTO , CA
94303

TITLE

Body fluid sampler

FILING FEE	FEES: Authority has been given in Paper No. _____ to charge/credit DEPOSIT ACCOUNT No. _____ for following:	<input type="checkbox"/> All Fees <input type="checkbox"/> 1.16 Fees (Filing) <input type="checkbox"/> 1.17 Fees (Processing Ext. of time) <input type="checkbox"/> 1.18 Fees (Issue)
RECEIVED		

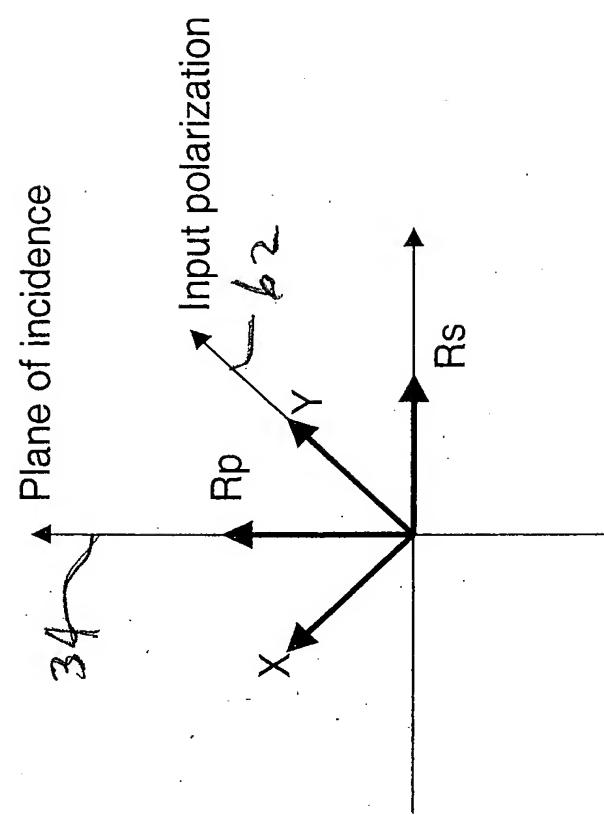
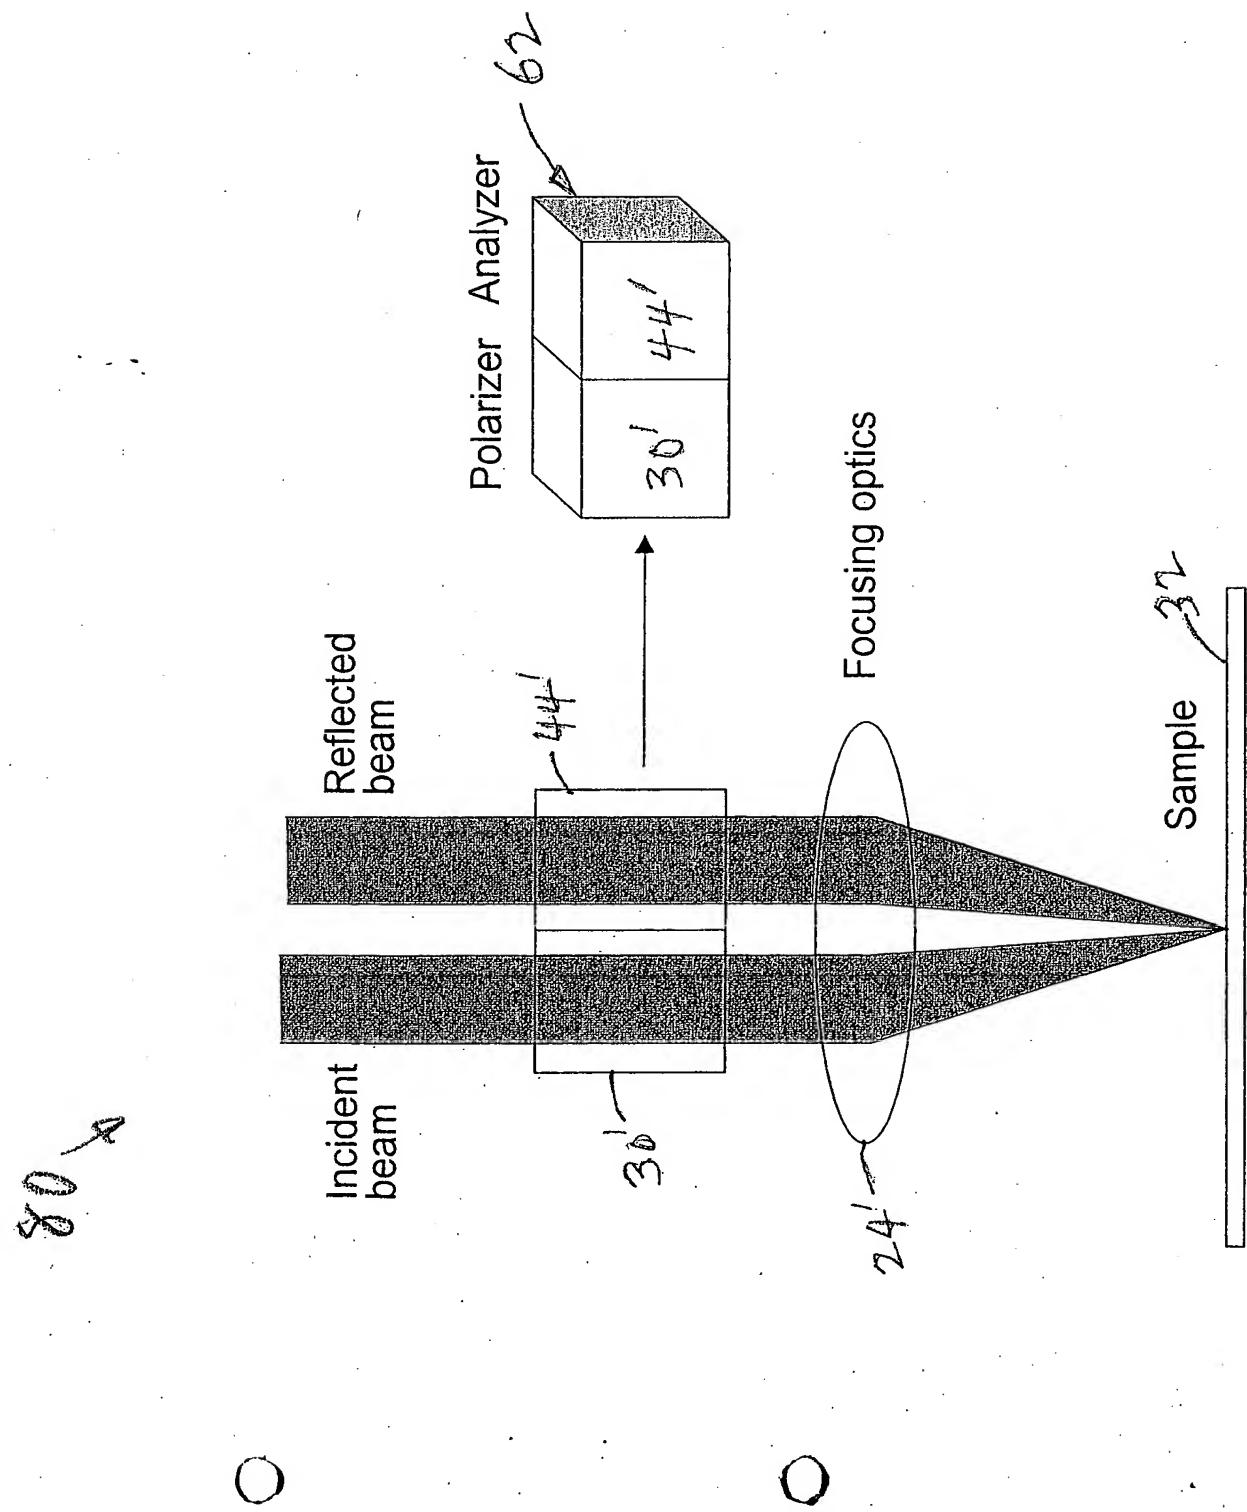


Fig 1B

Fig. 1C



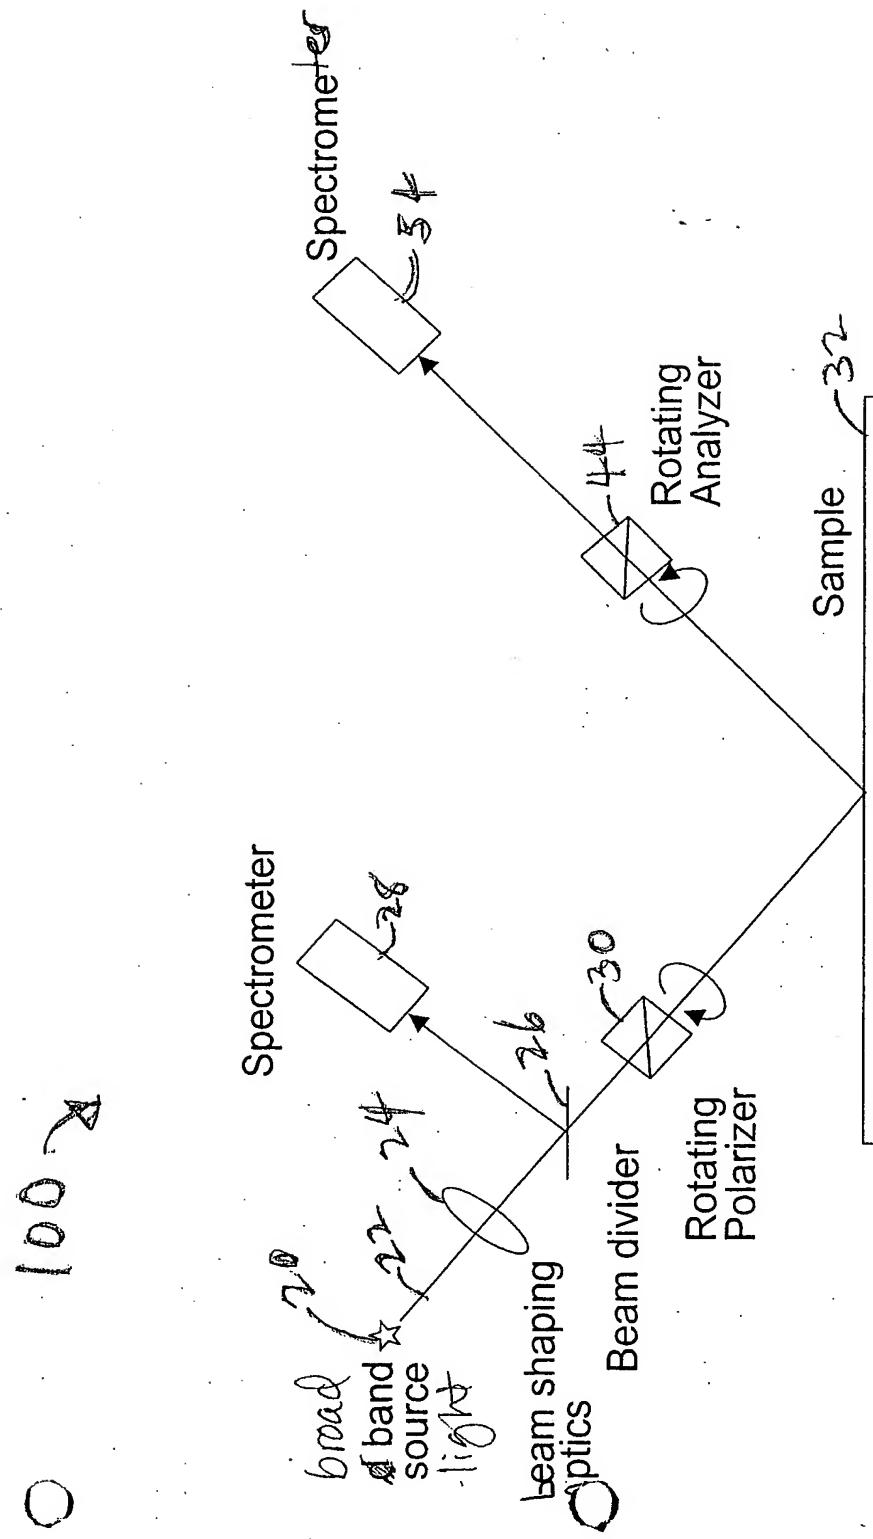


Figure 2. Ellipsometer or reflectometer with rotating polarizer and analyzer

Fig. 3

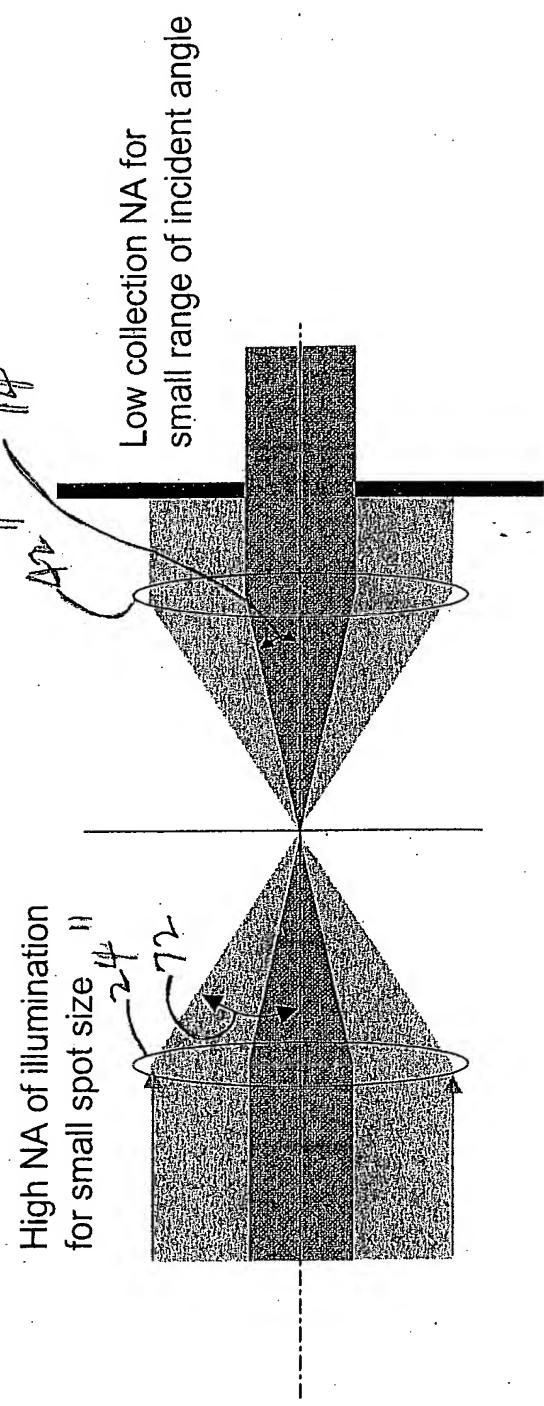
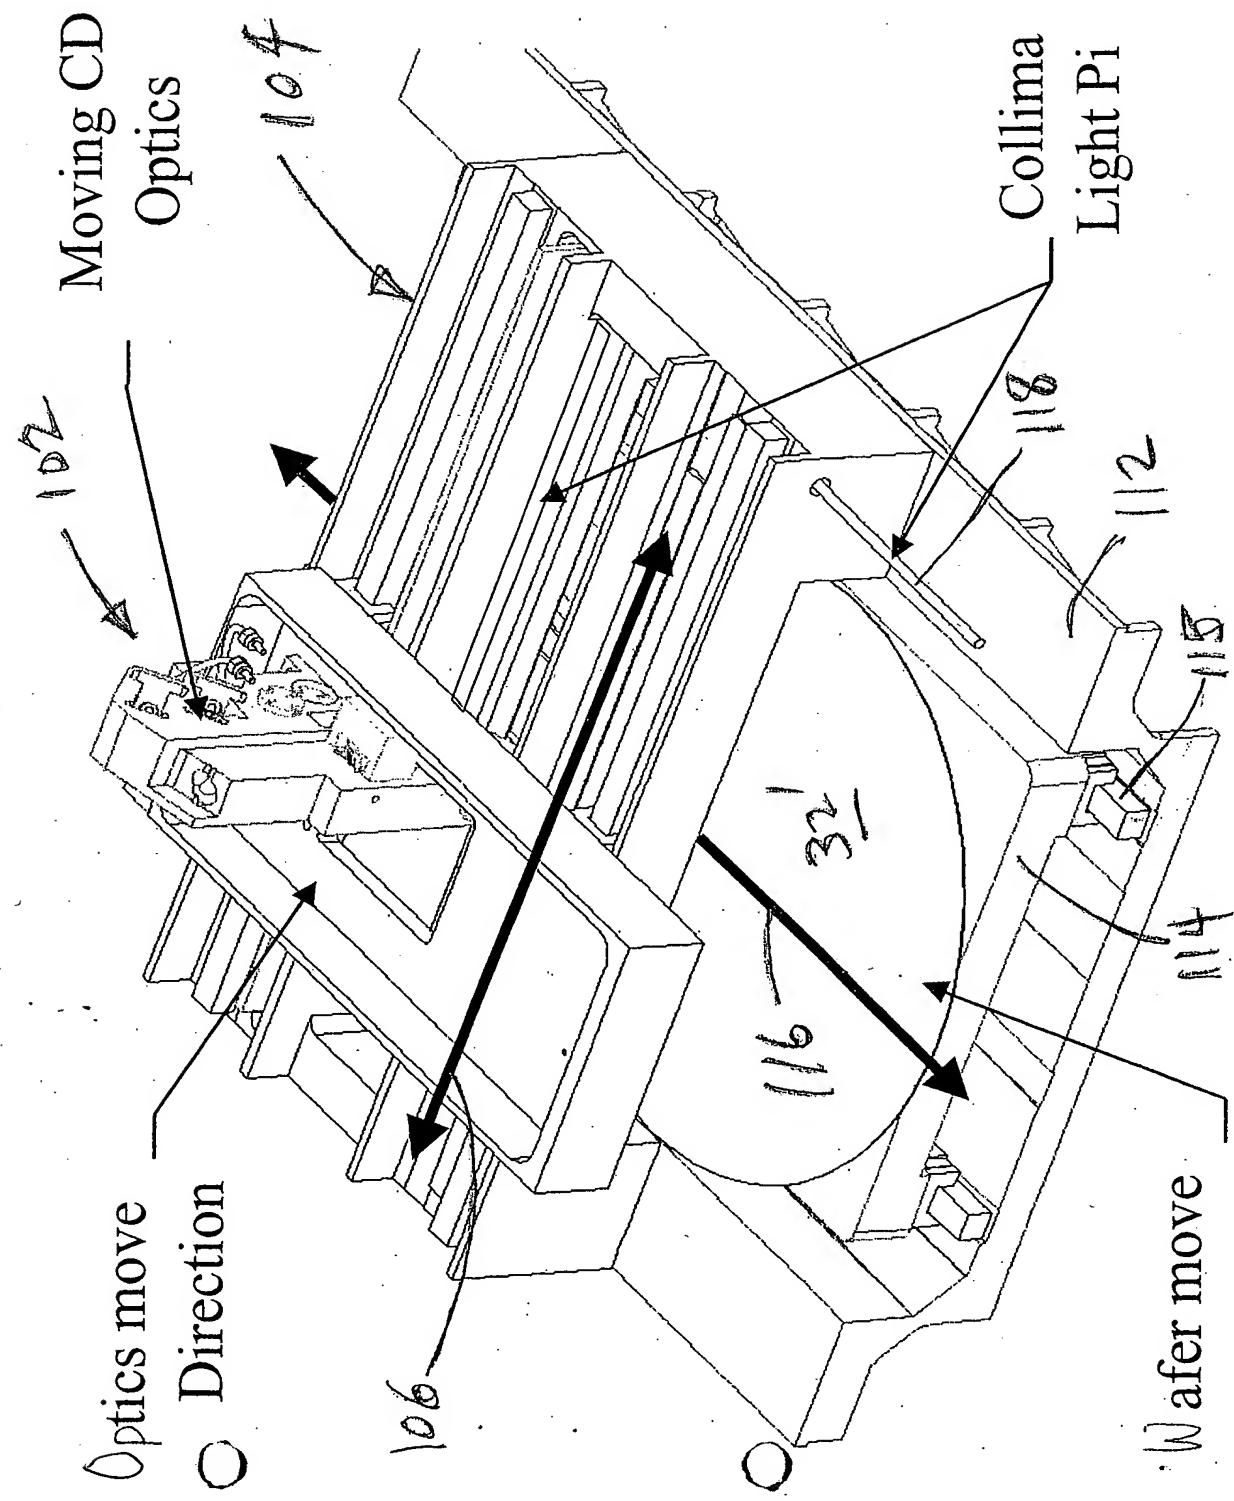


Figure 2a: Asymmetric NA for illumination and collection.
Shown in transmission mode, can be applied to reflection mode.

Fig. 4A



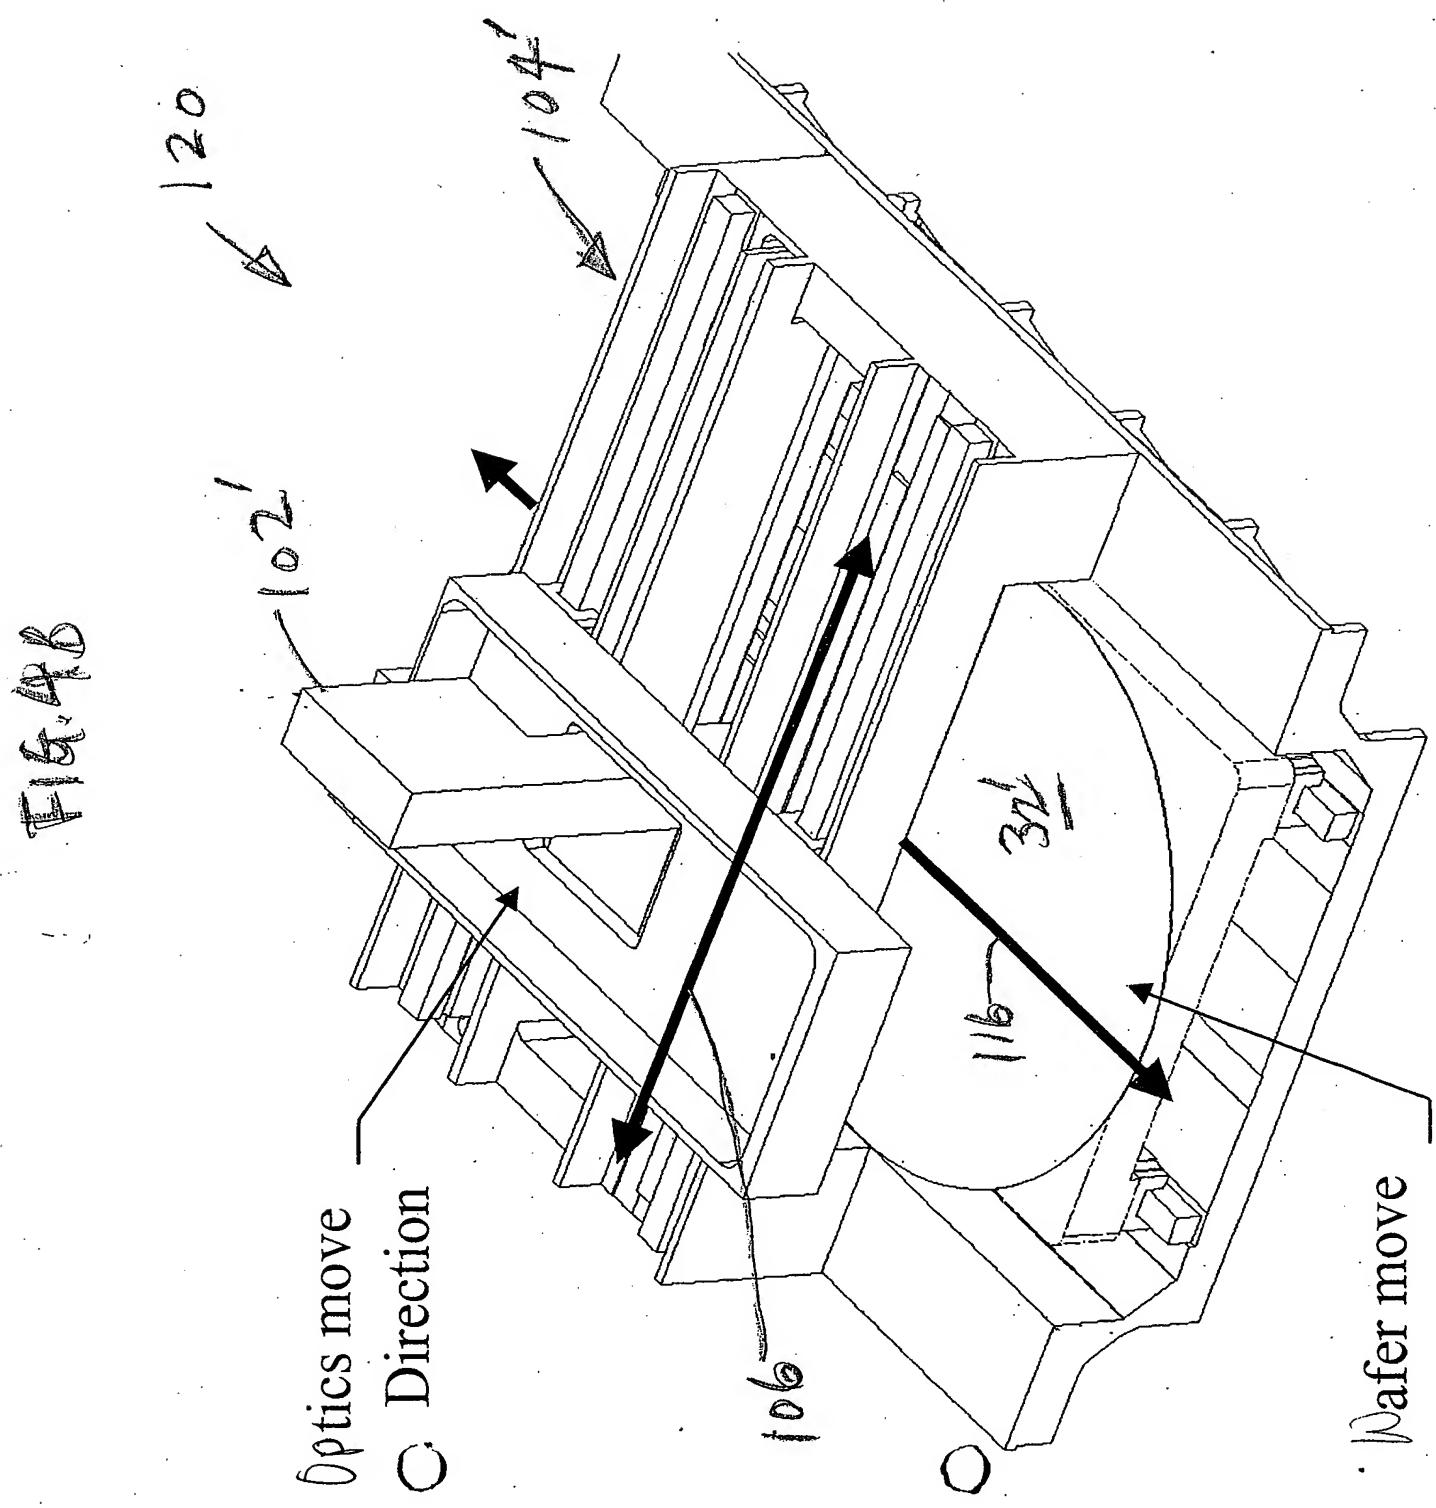
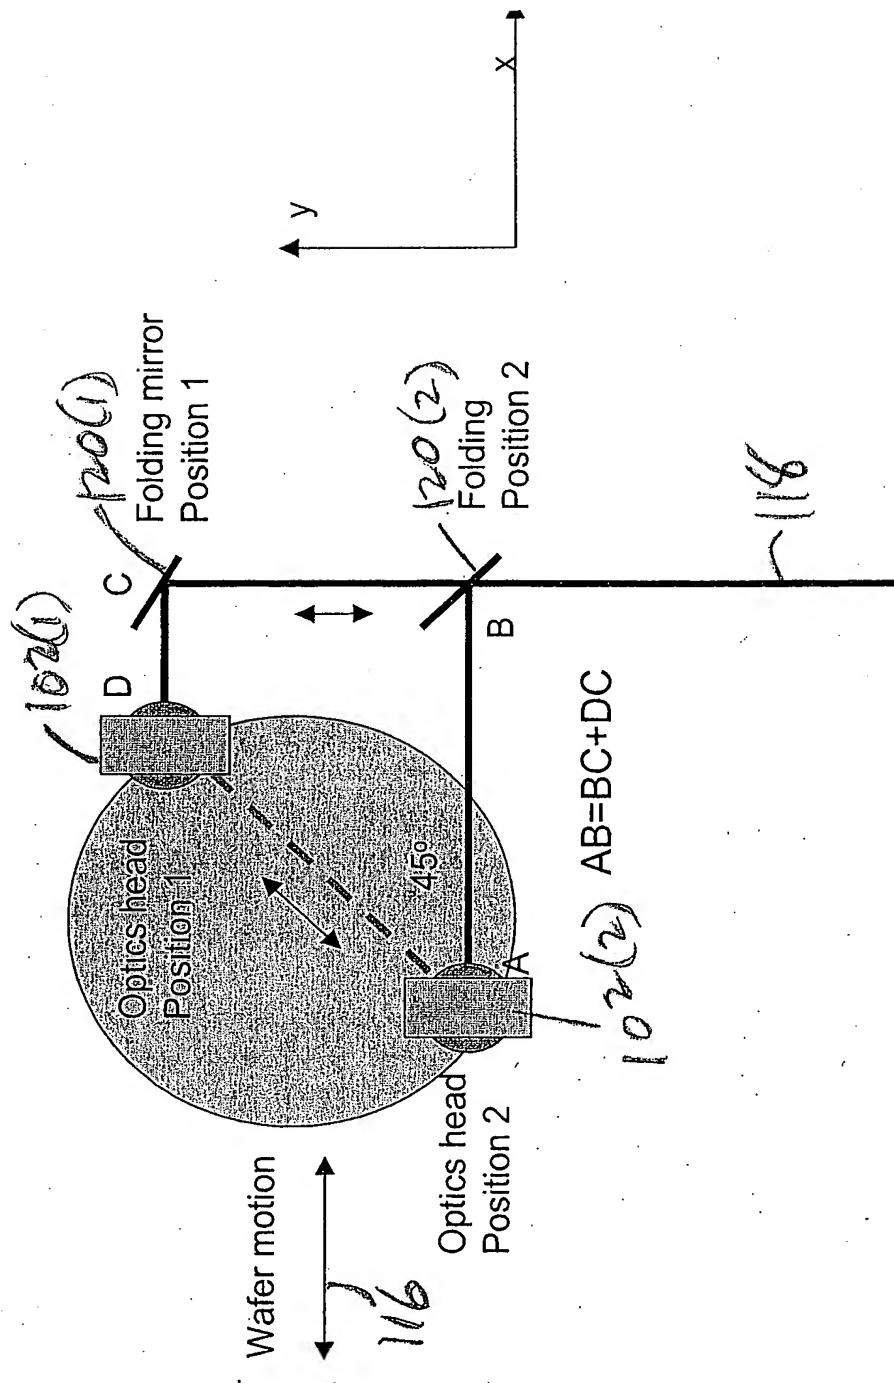
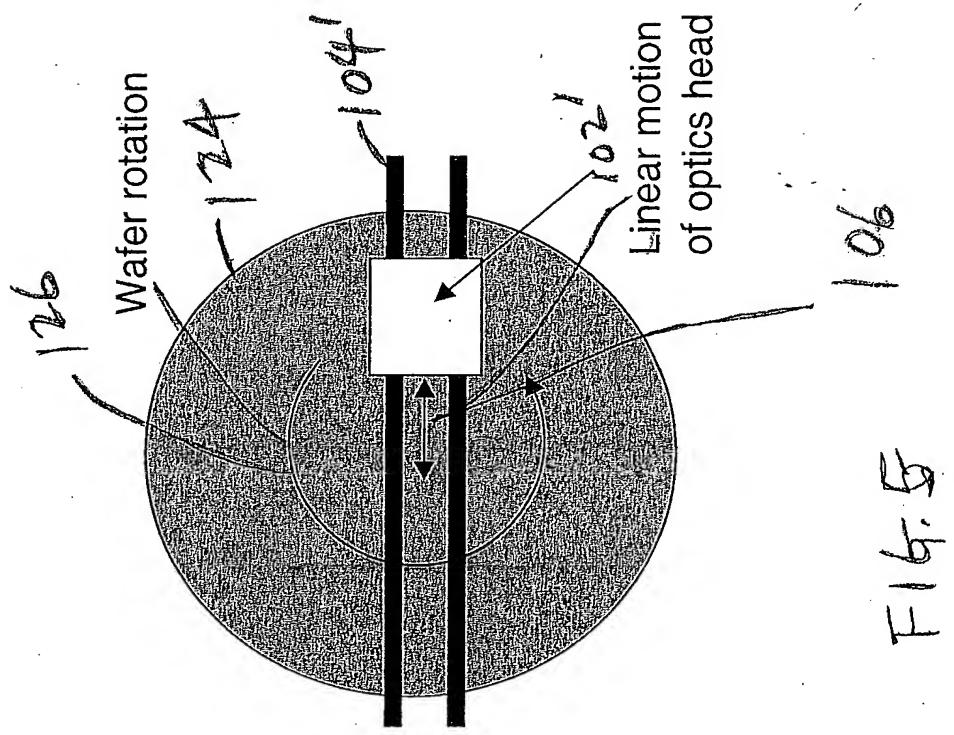


Fig. 4c





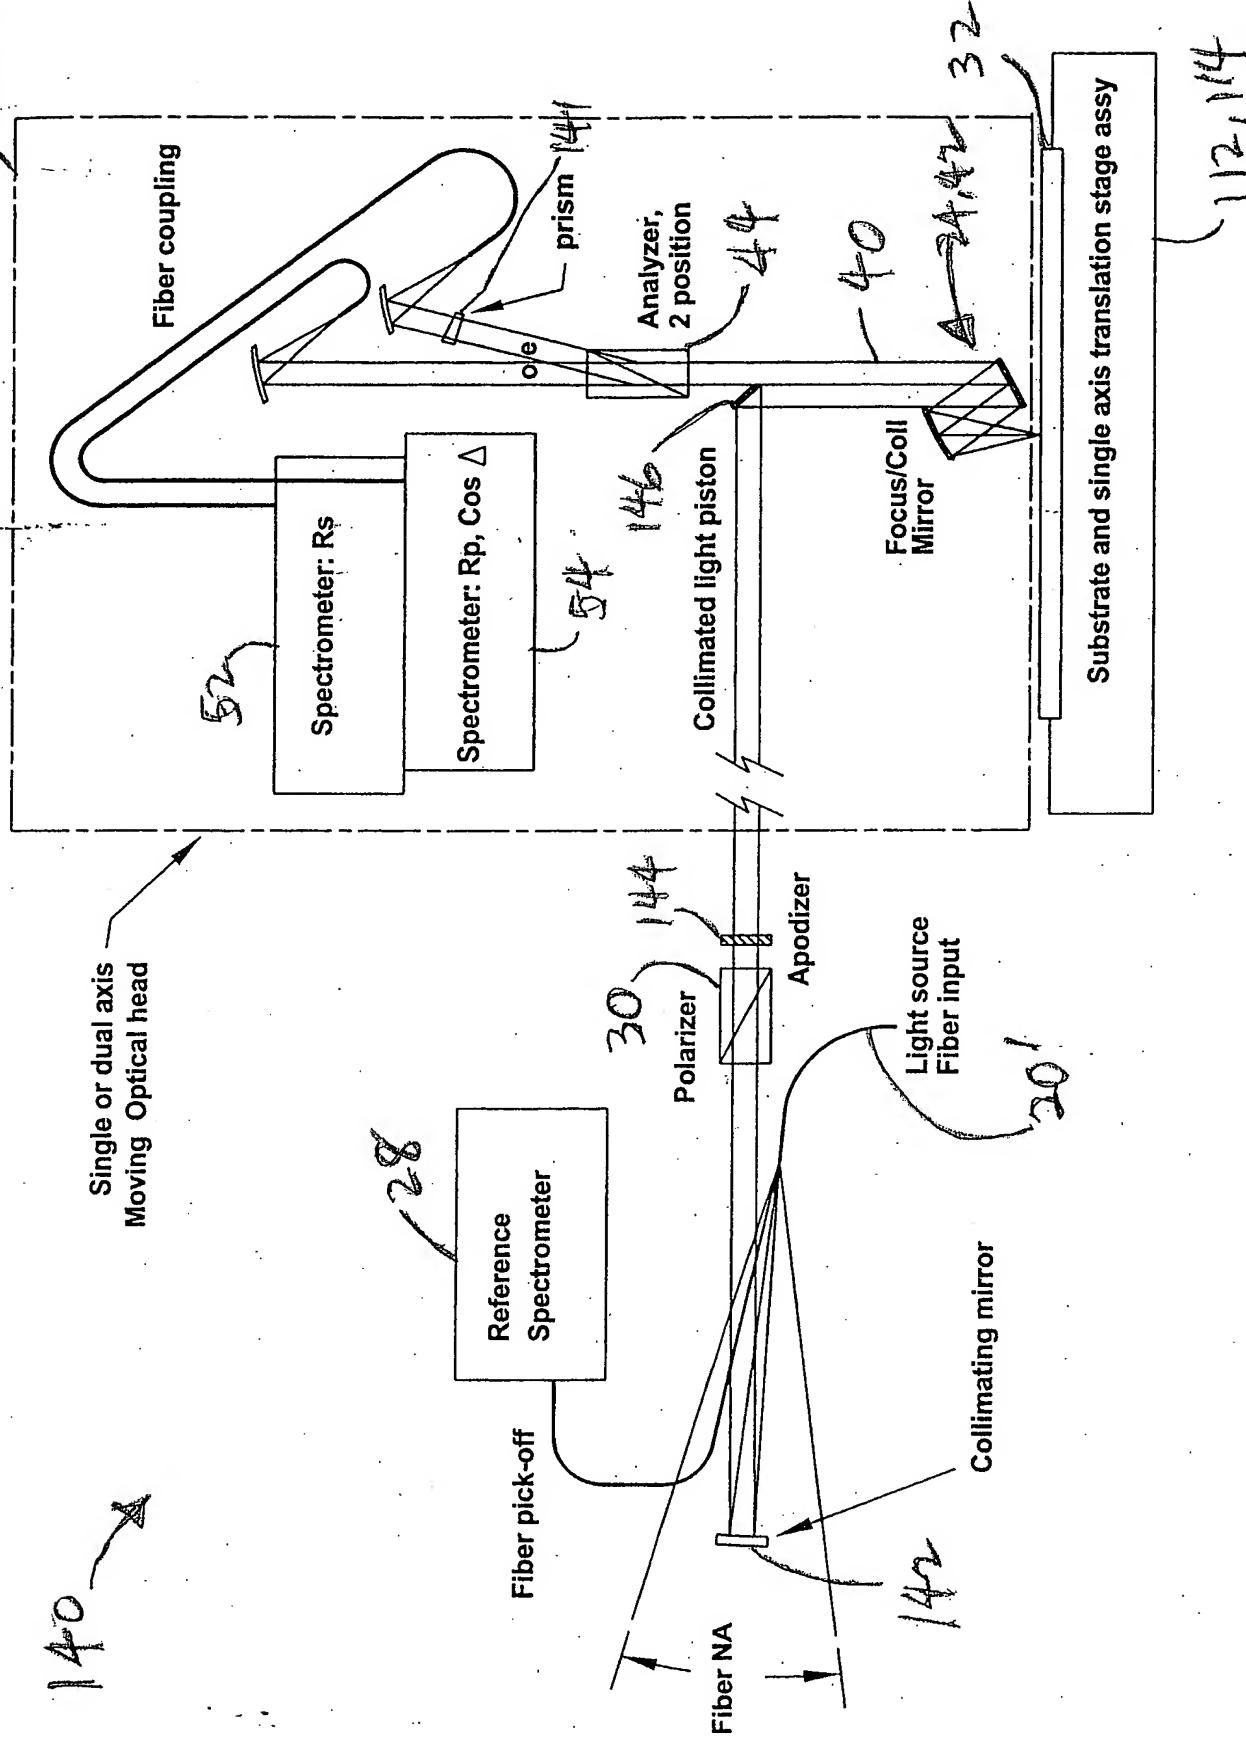


Fig. 6

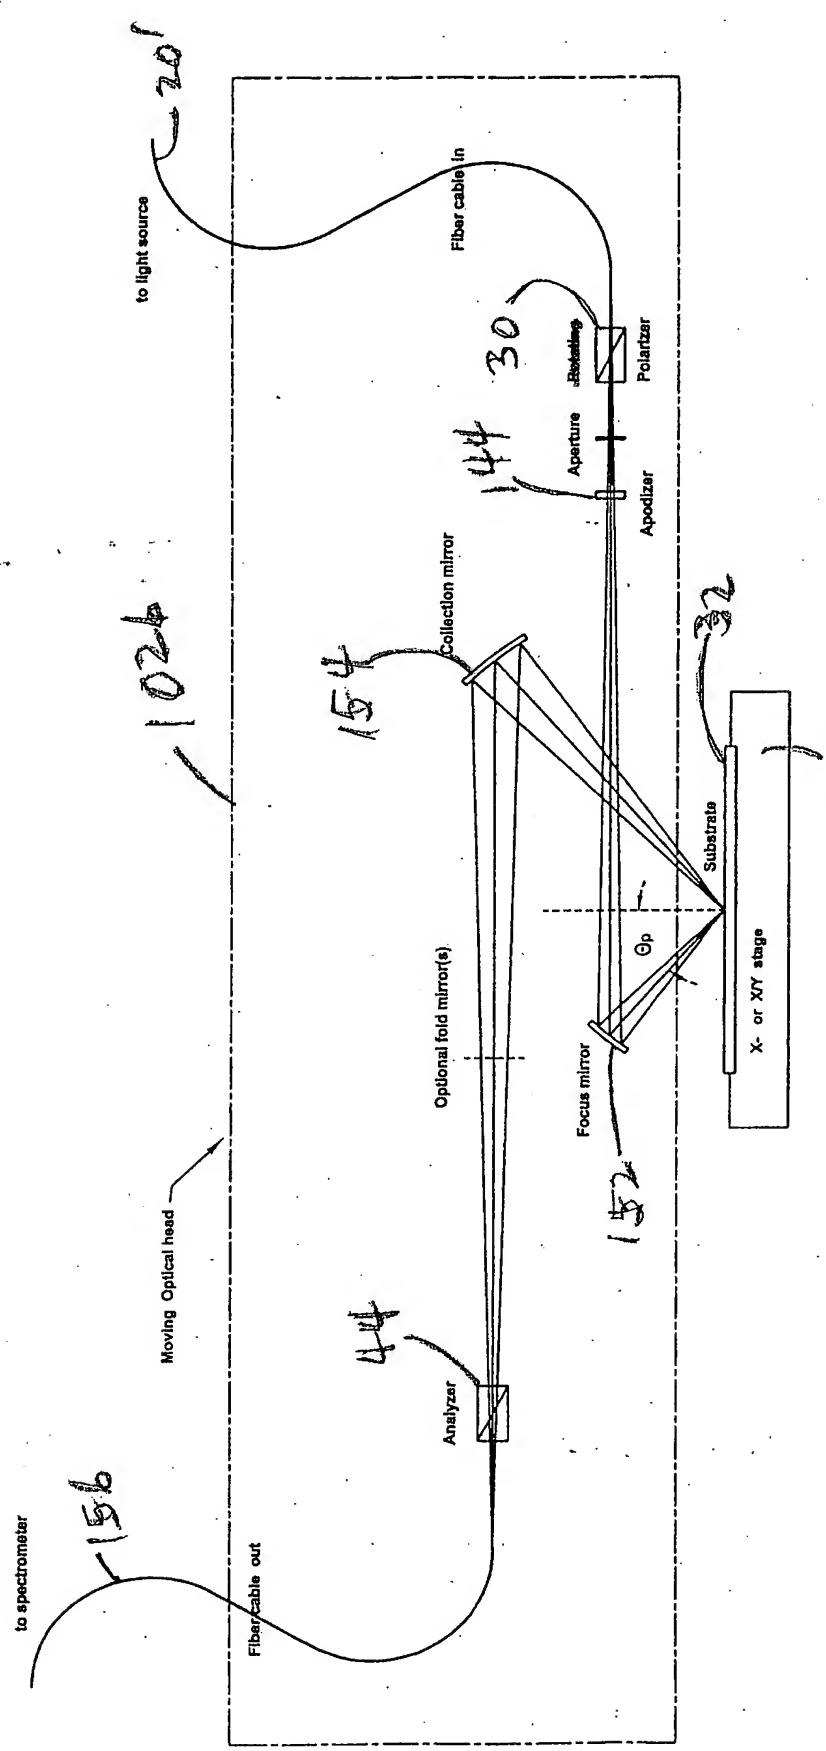


Fig. 7

148

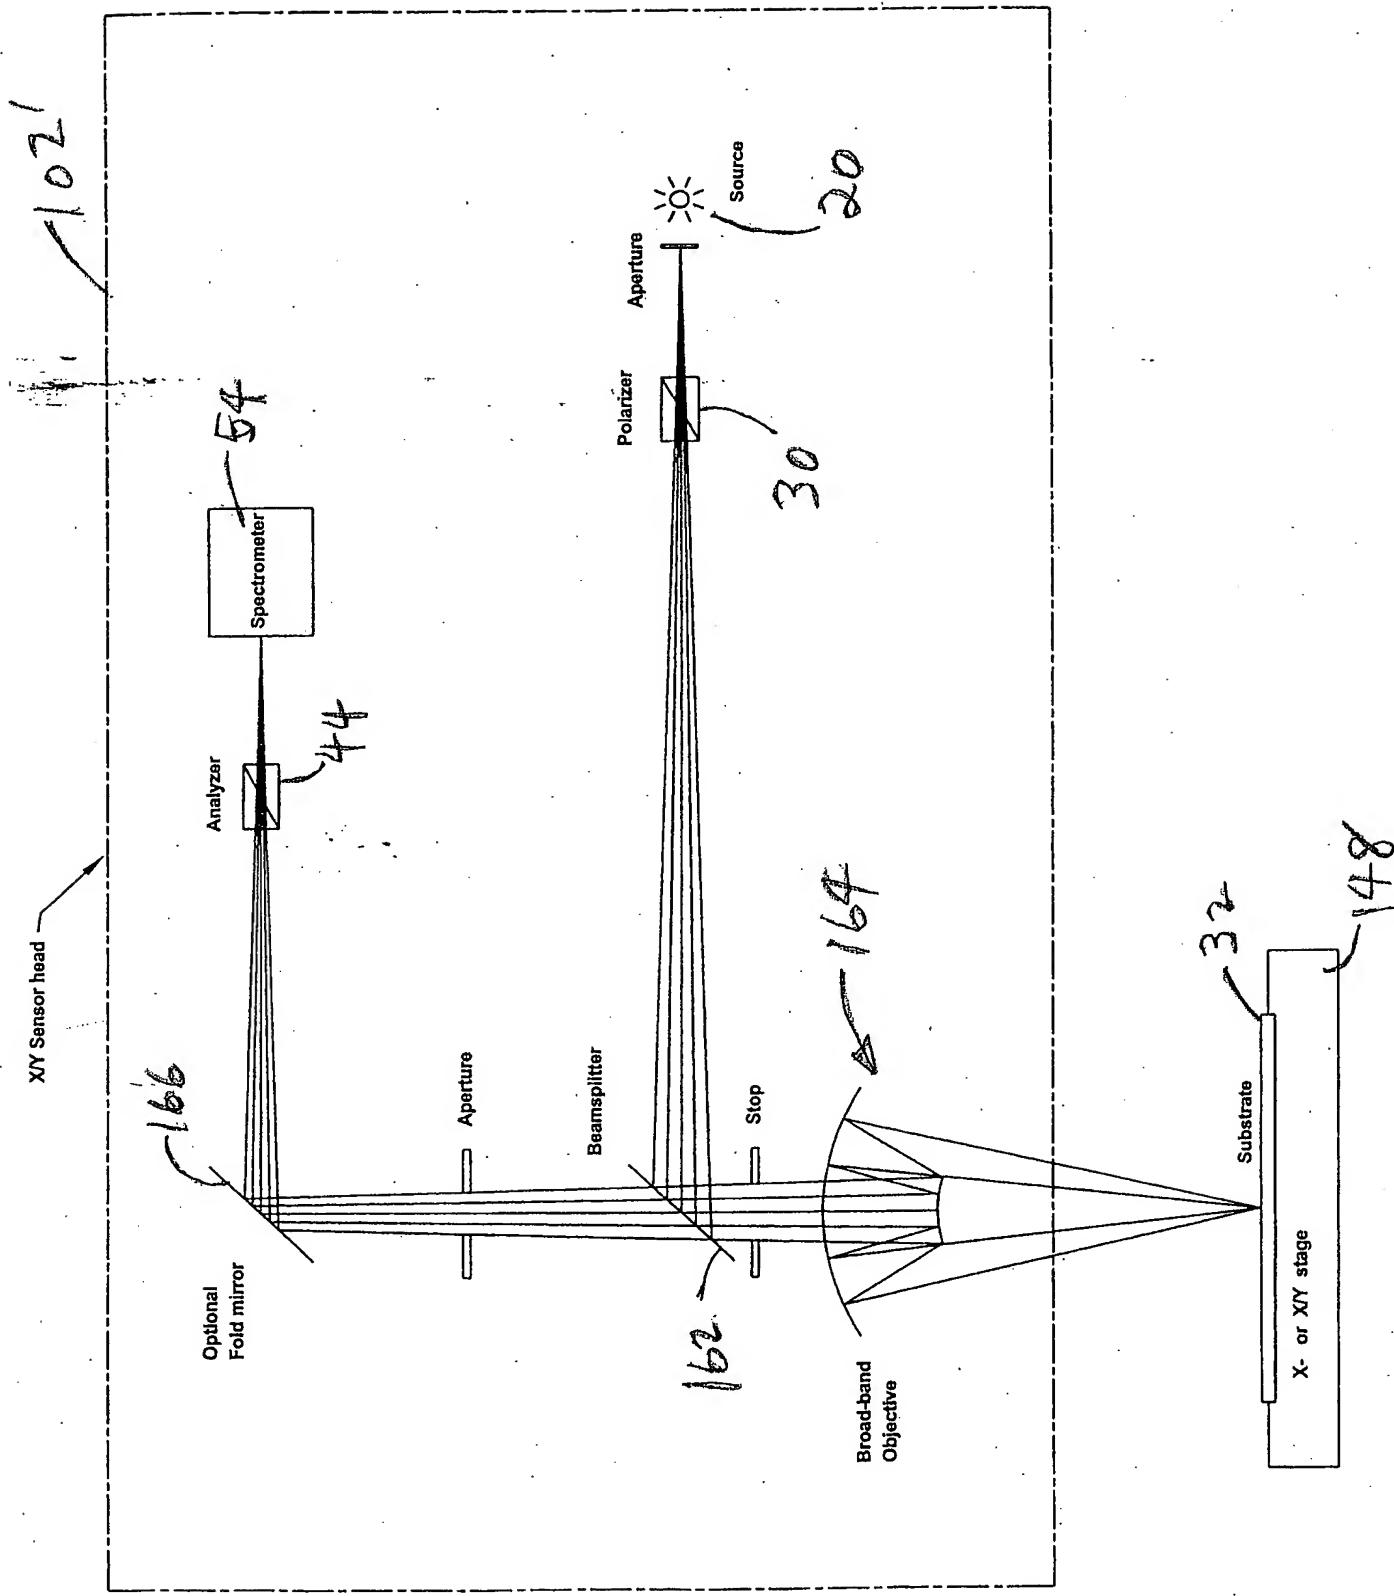
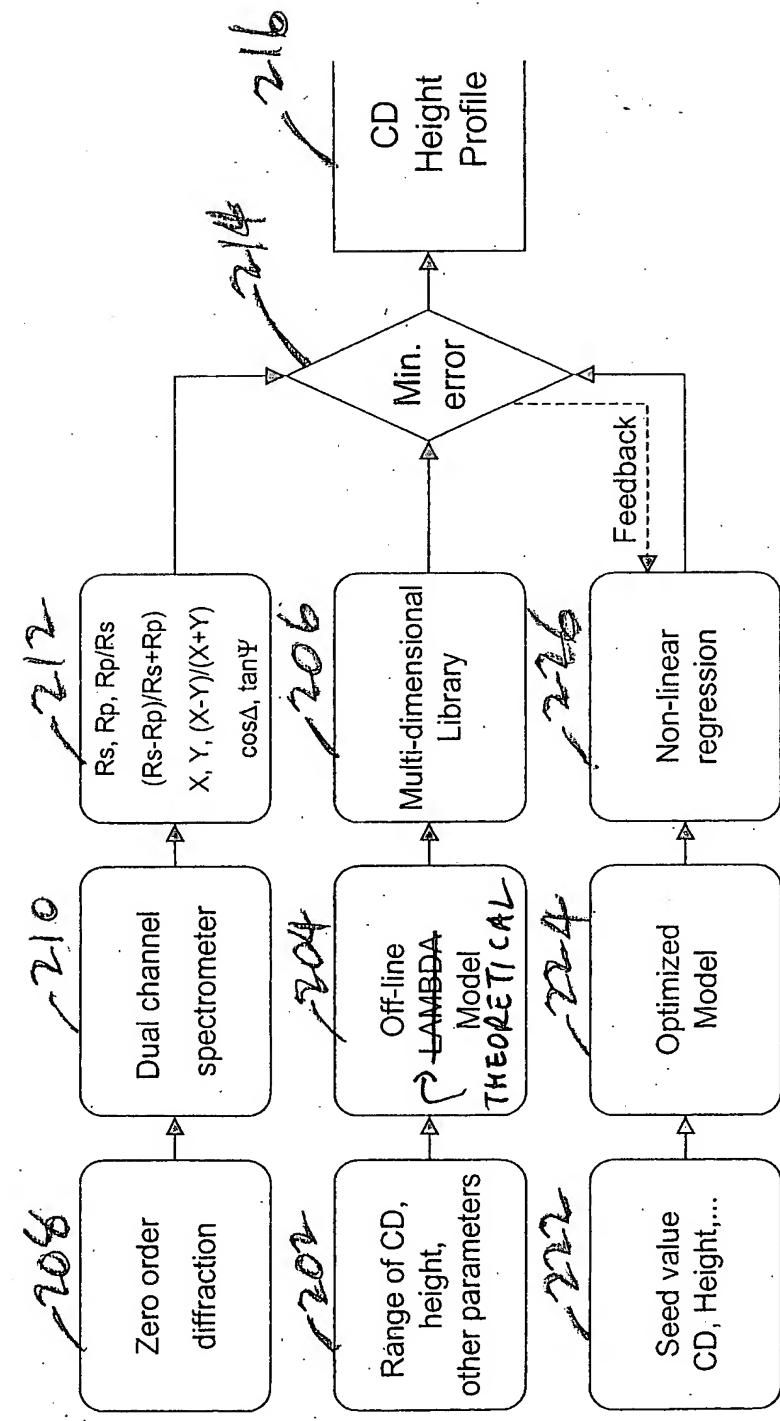


Fig. 8

Fig. 9



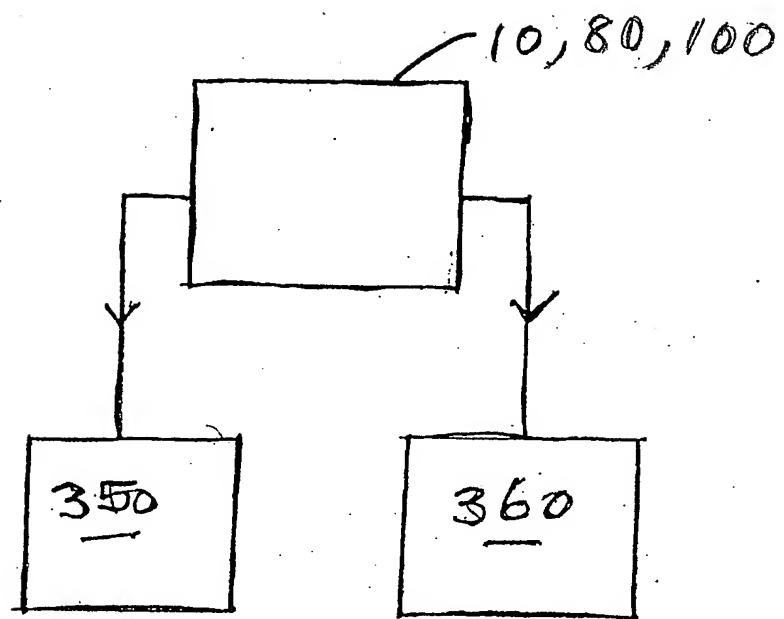



FIG. ~~10~~ 10

Fig. 11

350

Points of Integration

iFilm (Feed Forward)




iMacro (Feed Forward or Scrap)

352
354

356

358

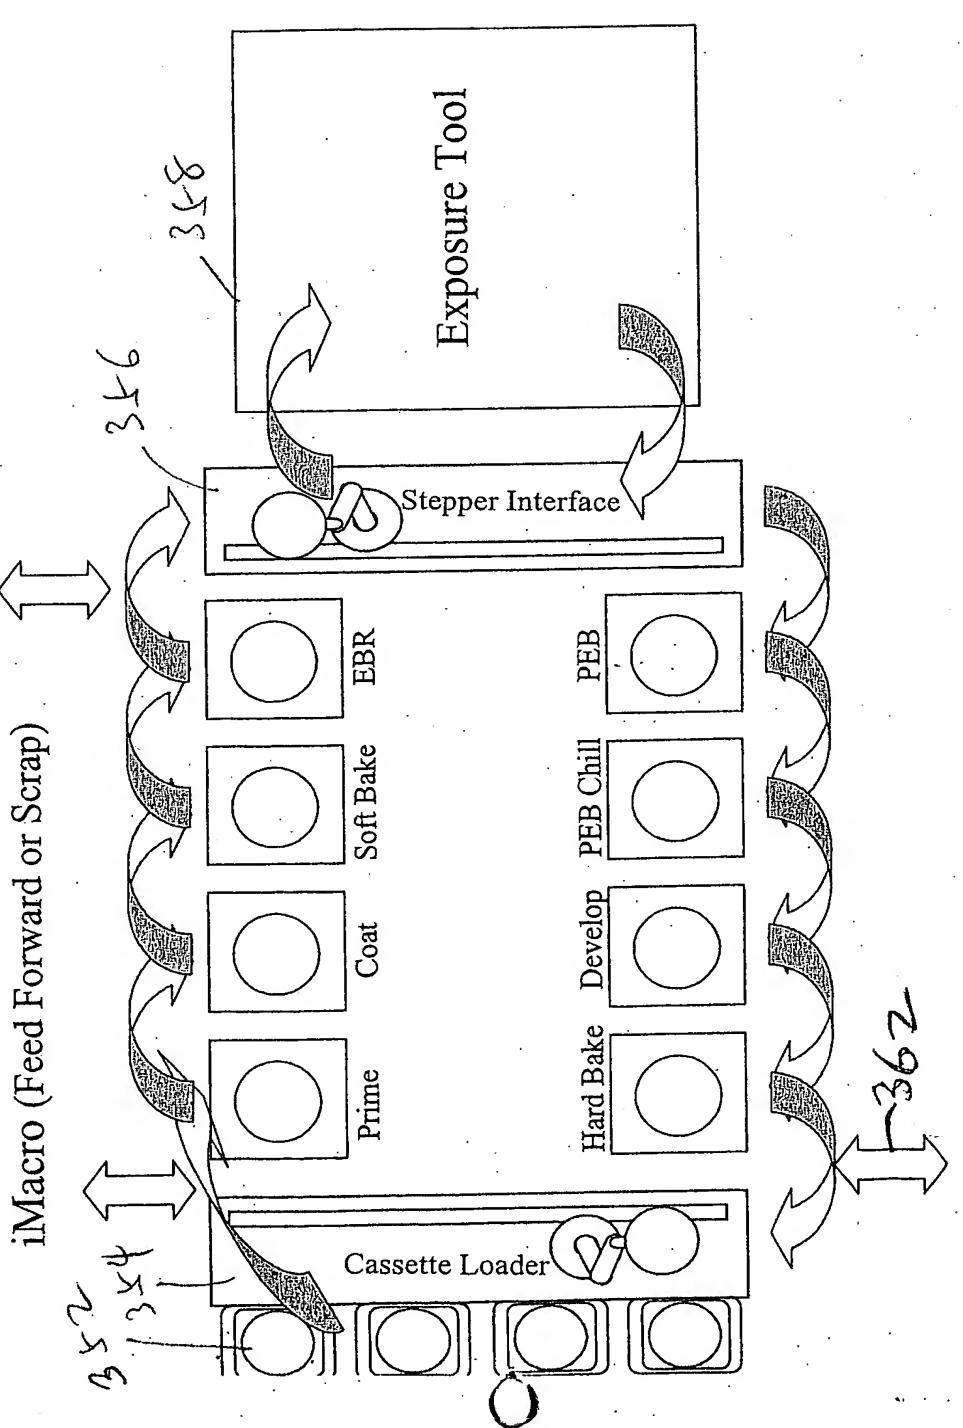

ICD (Feed Forward/Back)